


# DATA SHEET

## S4LFT1330/373

F-Theta  
standard - fused silica  
420 - 480 nm



### outline drawing

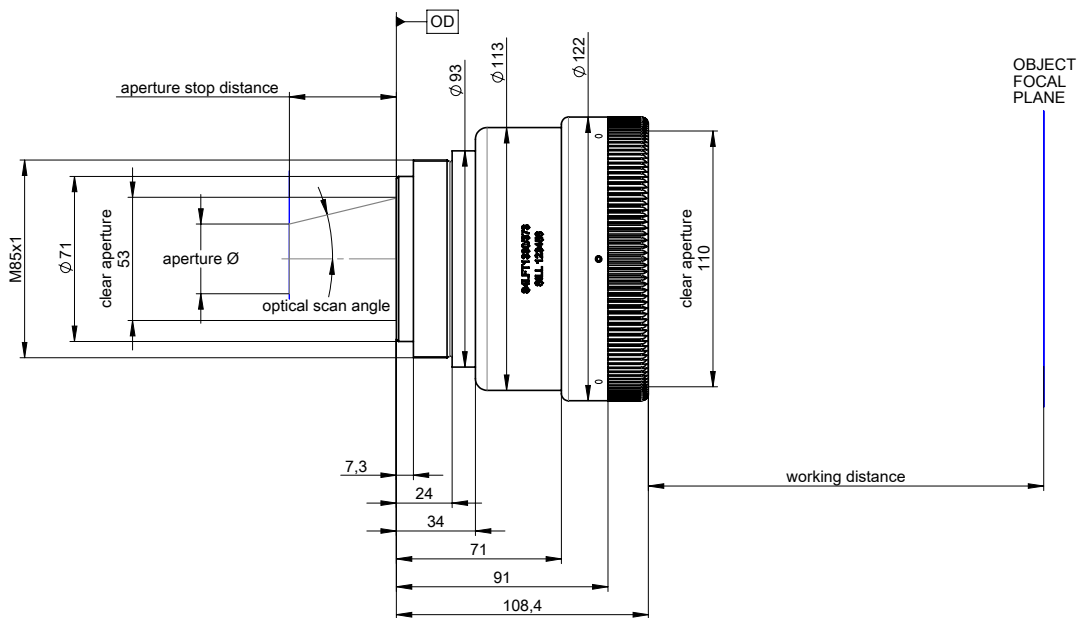


# DATA SHEET

## specifications

article number	S4LFT1330/373	
design wavelength [nm]	450	
effective focal length [mm]	338.9	
max. entrance beam-Ø [mm]	20.0	30.0
aperture stop distance [mm]	37.5	46.0
working distance [mm]	270.1	270.0
scan area for a 2 mirror system with mirror distance from lens housing for mirror 2 / mirror 1	180 x 180	115 x 115
	25.0 / 51.0	28.0 / 64.0
max. telecentricity error [°]	11.1	11.2
total transmission [%]	> 98	
lens material	fused silica	
LIDT (coating)	not specified	
SP and USP usable	yes	
weight [kg]	1.5	
cover glass	S4LPG2175/373	
absorption [ppm]	not specified	
cleanliness	not specified	

## spot for 20.0 mm beam diameter

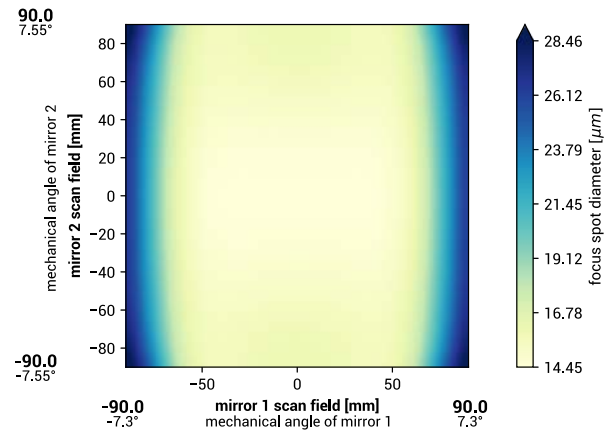


spot diameter at 86.5 % level for a Gaussian beam ( $M^2 = 1$ ) with 20.0 mm diameter at  $1/e^2$ , clipped at 20.0 mm field size and mirror distances as given above for a two mirror scan system

## back reflection position

back reflections [mm] for 450	
3.70	
38.60	
113.70	
115.20	
177.20	
0.00	
0.00	
0.00	
0.00	
0.00	

## spot for 30.0 mm beam diameter

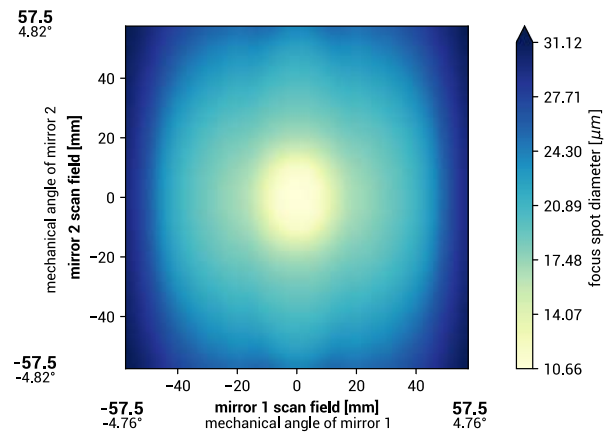

spot diameter at 86.5 % level for a Gaussian beam ( $M^2 = 1$ ) with 30.0 mm diameter at  $1/e^2$ , clipped at 30.0 mm field size and mirror distances as given above for a two mirror scan system

## remarks

- The stated values are based on a vignetting of less than 1 %.
- Effective focal length and working distance have tolerance of +/- 1.5 %.
- Absorption tolerance +/- 25 %. Absorption may increase. Correct cleaning establishes original condition.